

CUSTOMER:

P/N: 0310.120AL

REV.


APPROVED BY:

REVISIONS

REV.	DESCRIPTION	DATE
△		2014/02/25
△		2015/01/26
△	Tail to new structure, change approval print, update note 1	2017/02/20
△		
△		
△		

NOTES:


- △ 1. RoHS shown on the carton

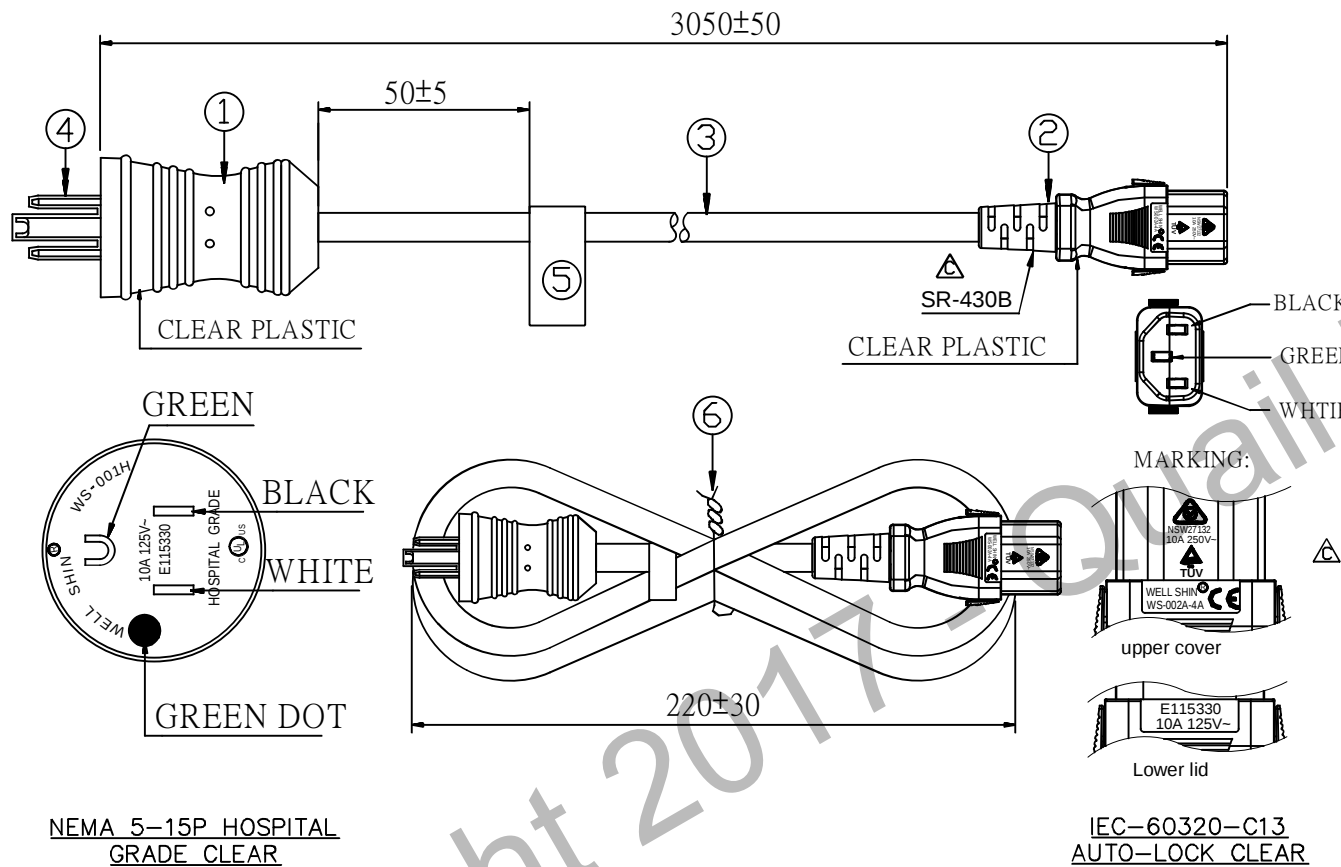

NEMA 5-15P HOSPITAL
GRADE CLEAR

IEC-60320-C13
AUTO-LOCK CLEAR

⑤ Hosp. Grade label

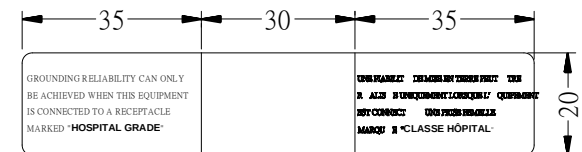

⑥	Cable tie	WHITE	1
⑤	Hosp. Grade label	---	1
④	PLASTIC CAP	WHITE	1
③	SJTW 18AWG*3C 105°C APPROVAL : UL,CSA	Patone Cool Grey 9C (GY-H)	1
②	WS-002A-4A 10 (A) 125 (V) APPROVAL : UL,CUL,SAA,TUV,CE	CLEAR	1
①	WS-001H 10 (A) 125 (V) APPROVAL : UL,CUL	CLEAR	1
ITEM	DESCRIPTION	COLOR	Q'TY

	SIGNATURE	QUAIL ELECTRONICS, INC. http://www.quail.com		
SAFETY ENGINEER:		PRODUCT NO:	001H+002A-4A	DATE: 2017/02/20
MANAGER BY:		UNIT:	mm	SHEET: 1 OF 1
CHECKED BY:		DWG NO:	0096-4266	REV. C
DRAWN BY:				